

FIG. 1

100

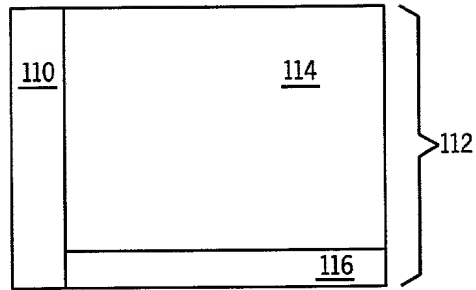


FIG. 2

100(a)



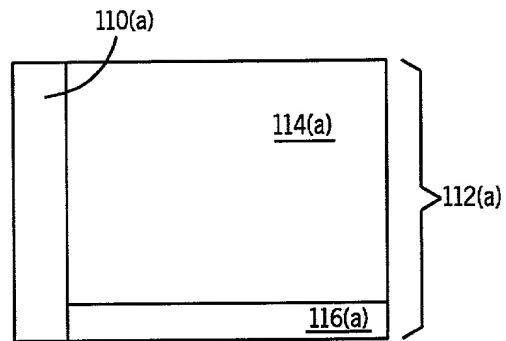


FIG. 3

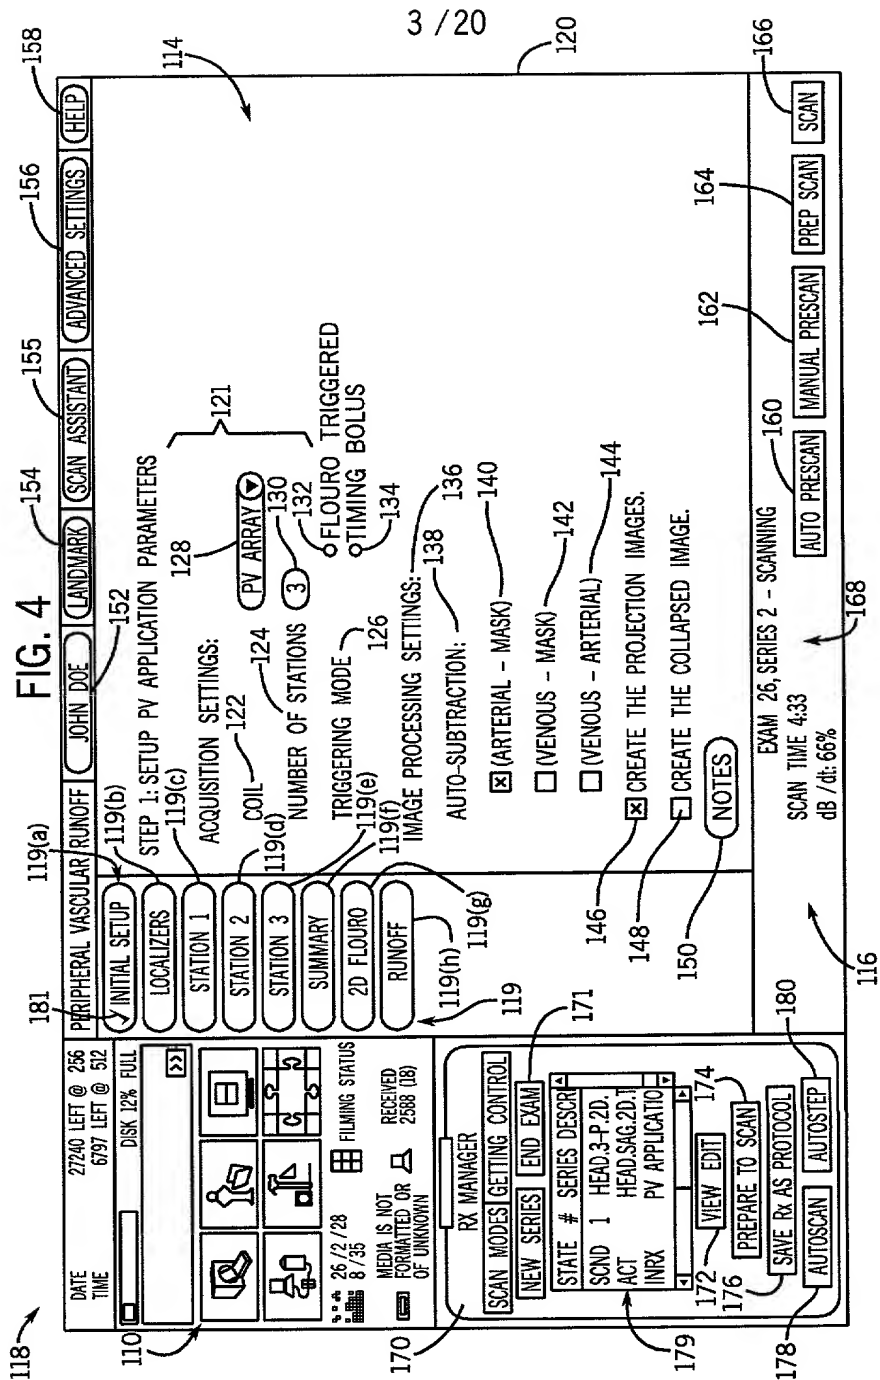

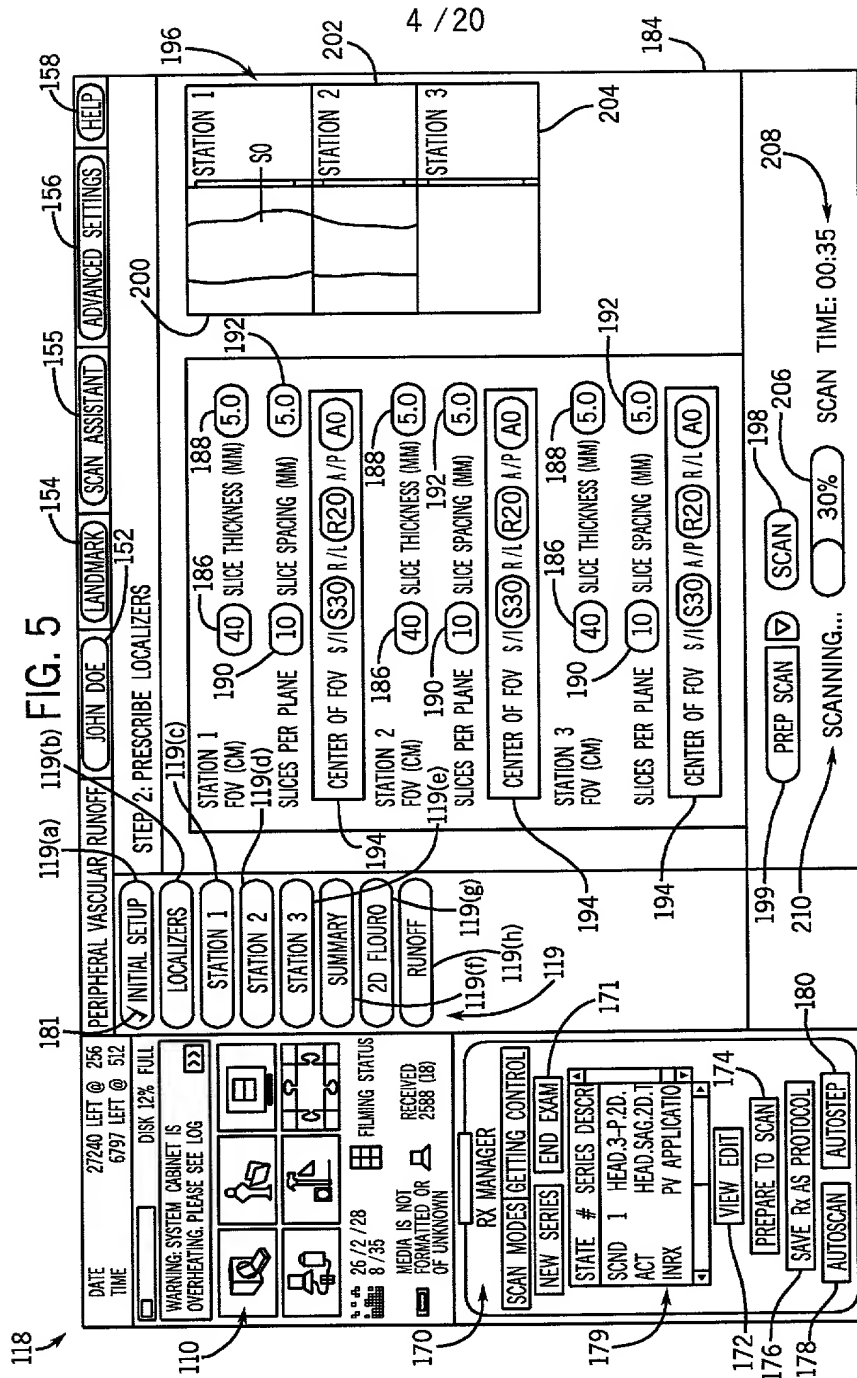

PATIENT INFORMATION

ACCESSION NUMBER 111222 214

PATIENT ID 33-22-4444 216

PATIENT NAME JOHN DOE 218

BIRTHDATE 9-22-1973 220 AGE 27 226

SEX M 222 WEIGHT 220 lb. 224 Kg. 232

RAD SMITH 228 REFER TIMBO 232

OPERATOR WILSON 230 STATUS NONE 234


EXAM DESCRIPTION PV RUNOFF 236

HISTORY 238

CLOSE 240

212

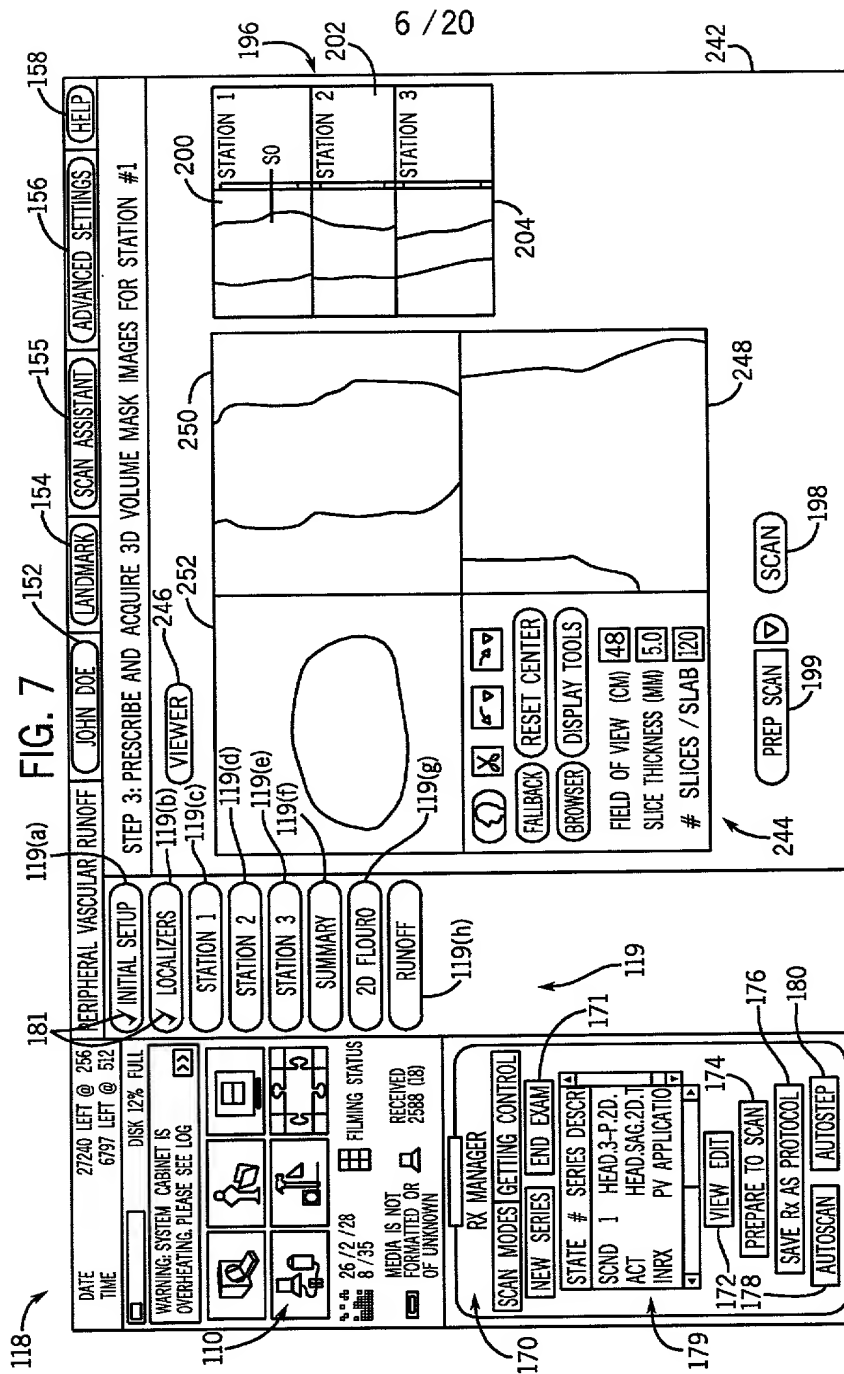FIG. 6



SCAN ASSISTANT

REQUESTED VALUE IS OUT OF RANGE.  
FIELD OF VIEW (cm):50

DEFAULT TO MAXIMUM VALUE OF 48.

OR

ENTER A NEW VALUE BETWEEN  
24 AND 48.

FIELD OF VIEW (cm): 48

ACCEPT CANCEL

FIG. 8

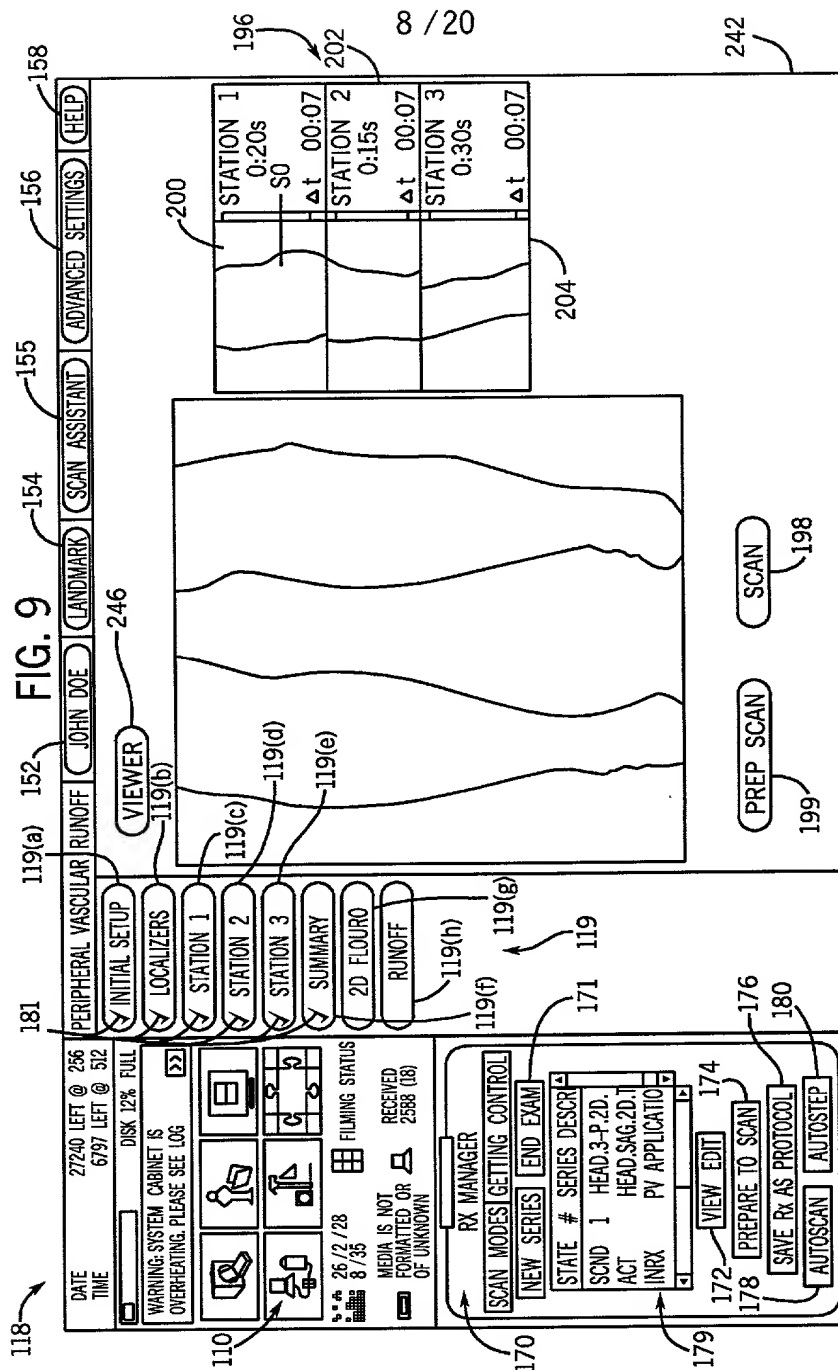
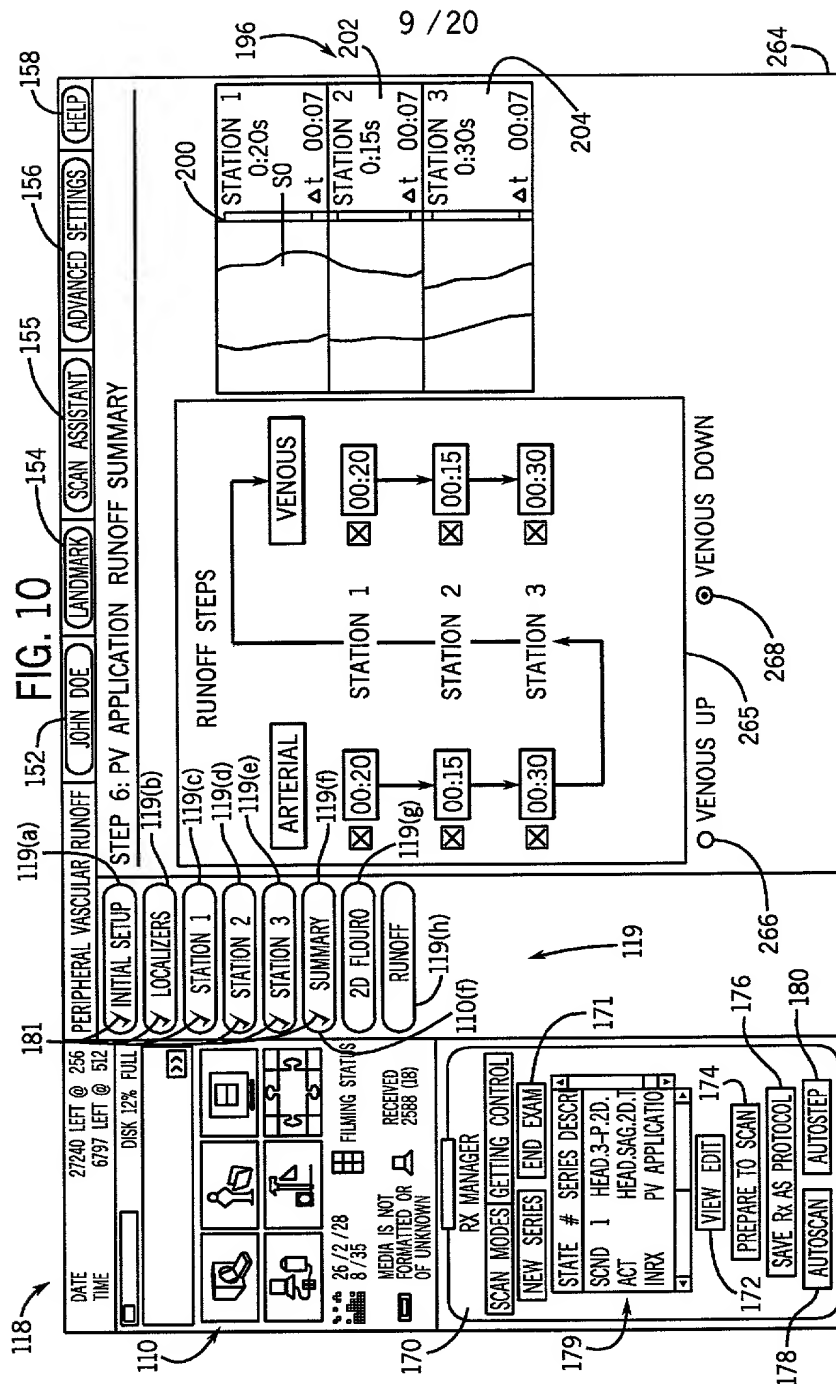
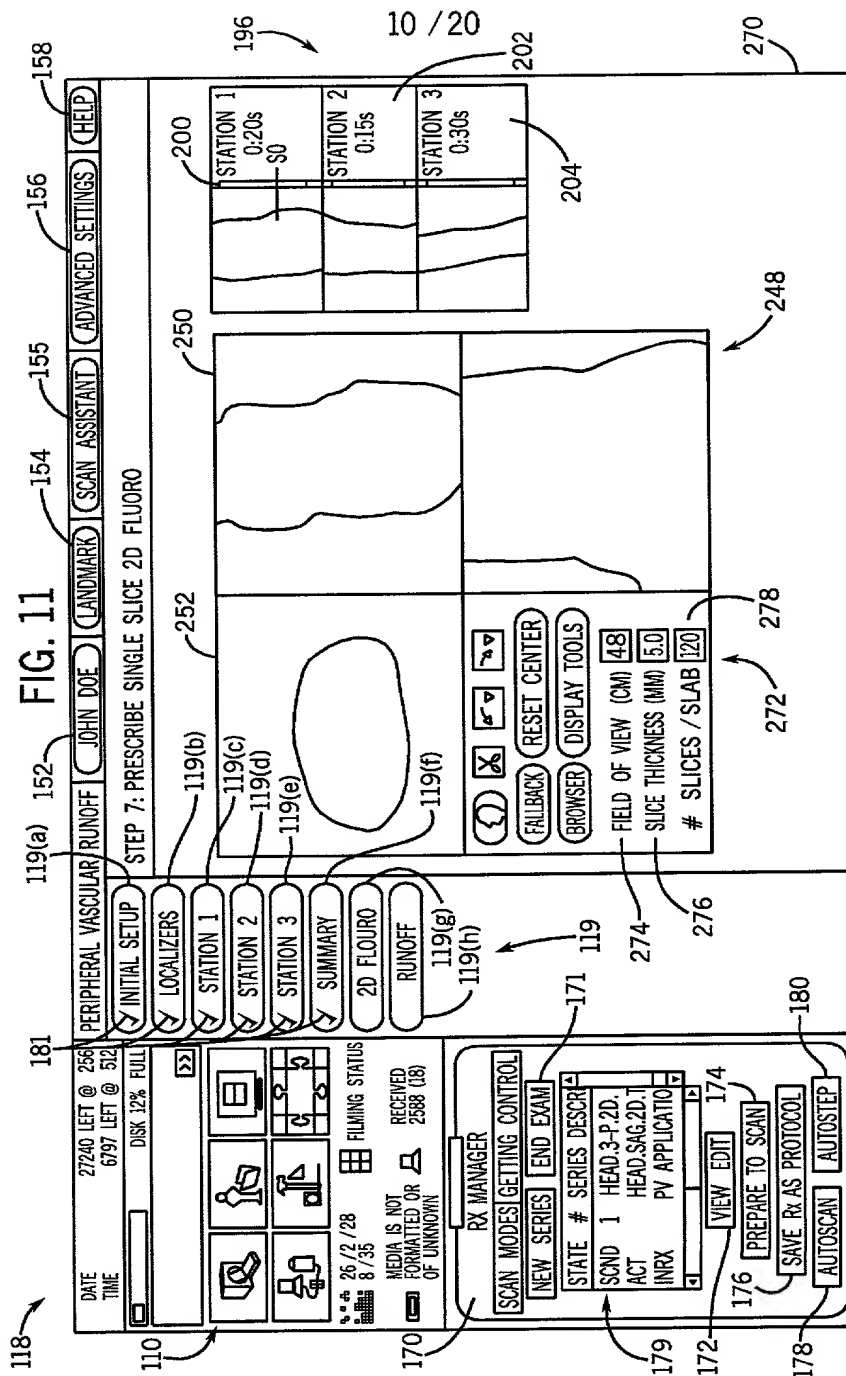
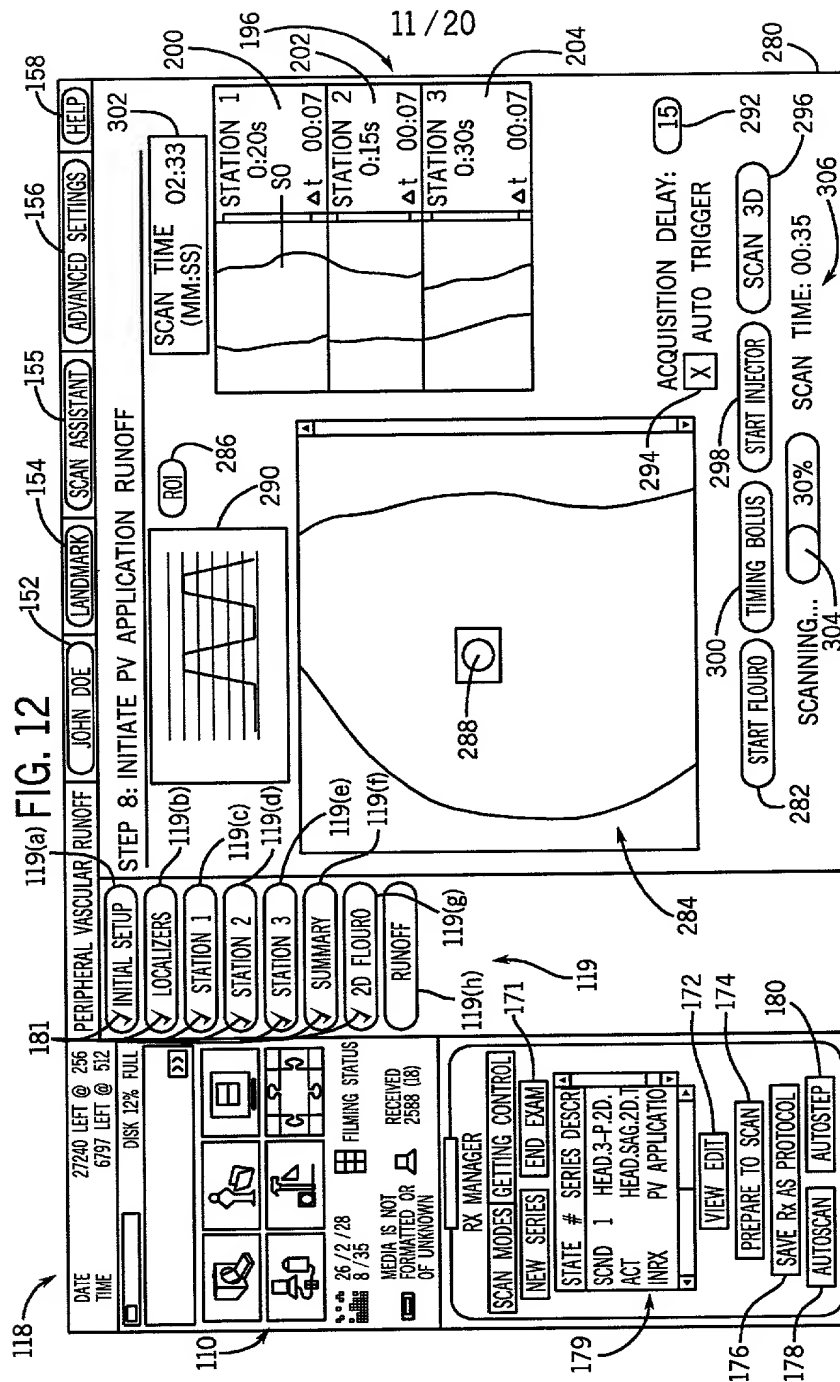


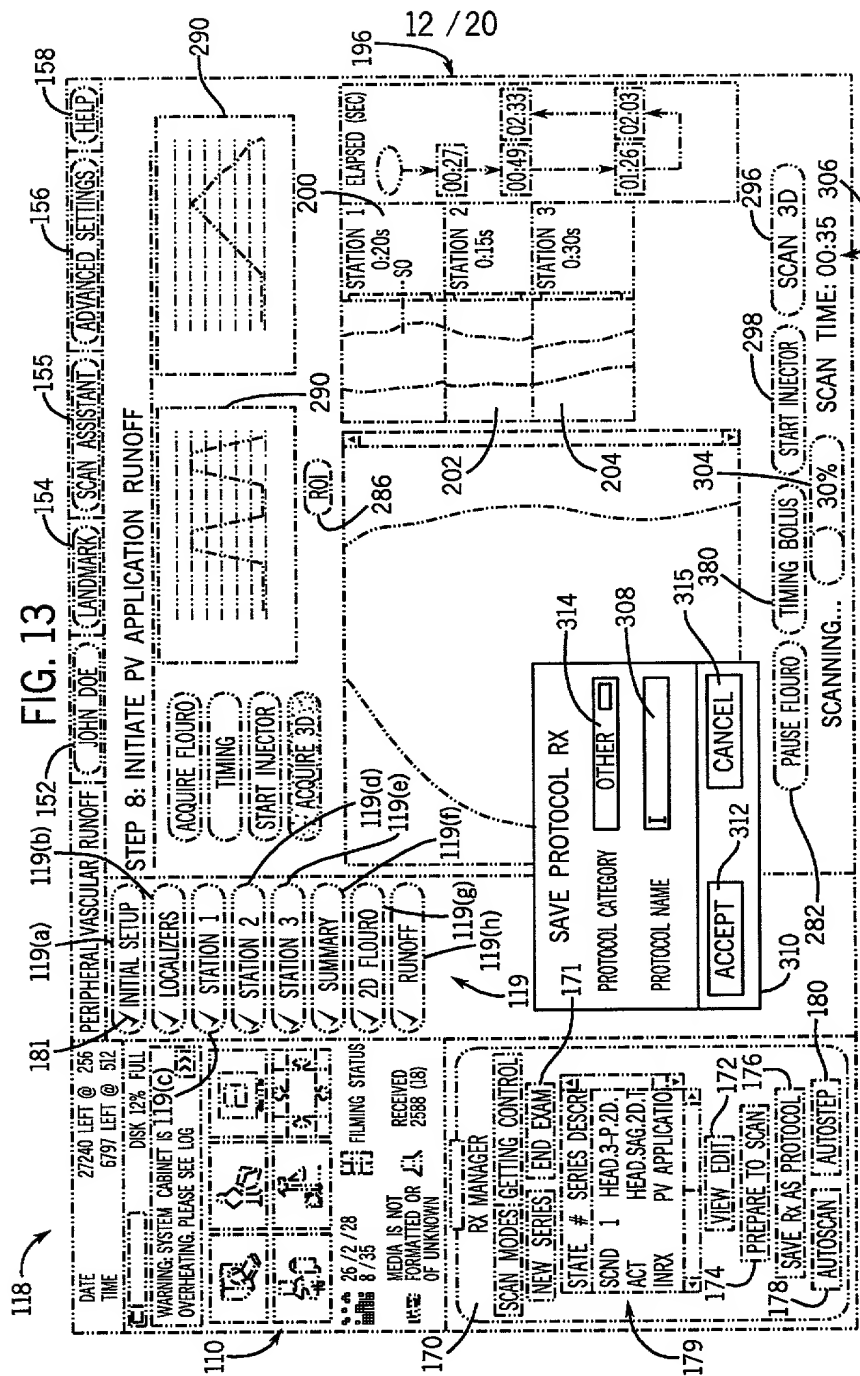


FIG. 10









316

ADVANCED SETTINGS

INITIAL SETUP:

PATIENT INFORMATION:

PATIENT HEIGHT (cm) 150 324

PATIENT POSITION SUPINE

PATIENT ENTRY FEET FIRST

POST PROCESSING SETTINGS

☐ MAGNITUDE SUBTRACTION

☒ COMPLEX SUBTRACTION 318

☒ COLLAPSE PROJECTIONS

☒ PROJECTION INCREMENT 320

☐ 19 PROJECTIONS @ 20 DEG. INCREMENTS

☐ 30 PROJECTIONS @ 10 DEG. INCREMENTS

☐ USER SPECIFIED

☐ AXIS OF ROTATION X-AXIS 328

CLOSE 326

FIG. 14

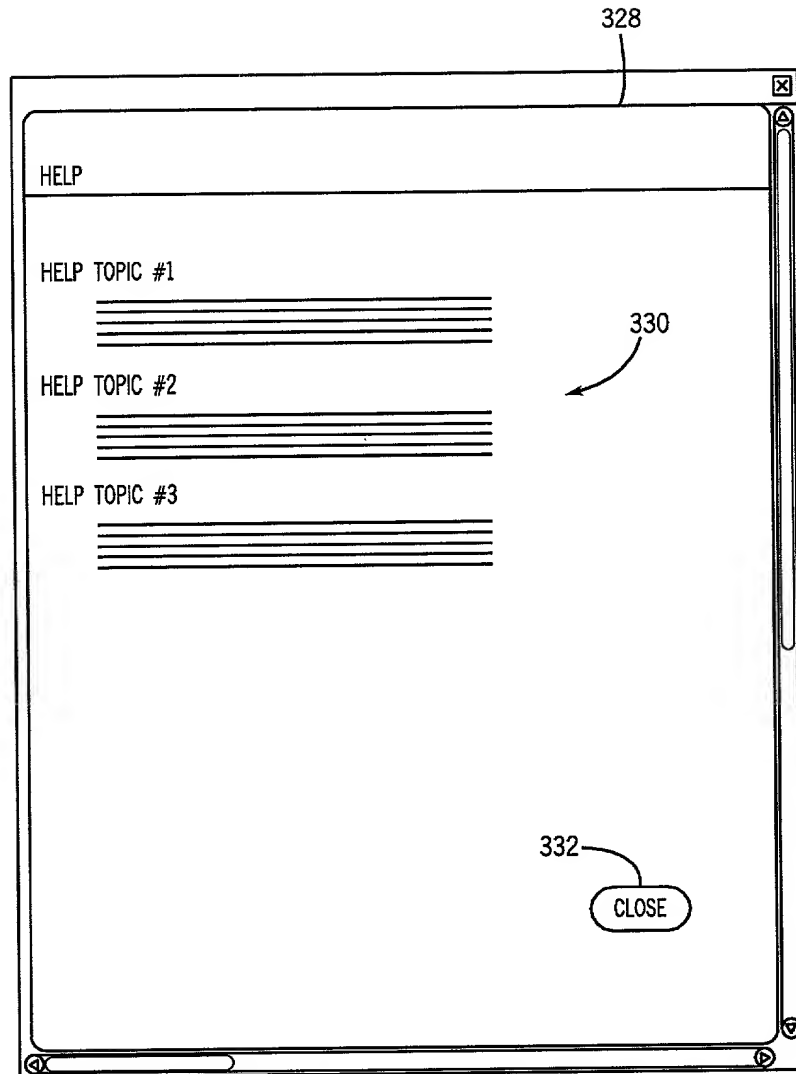


FIG. 15

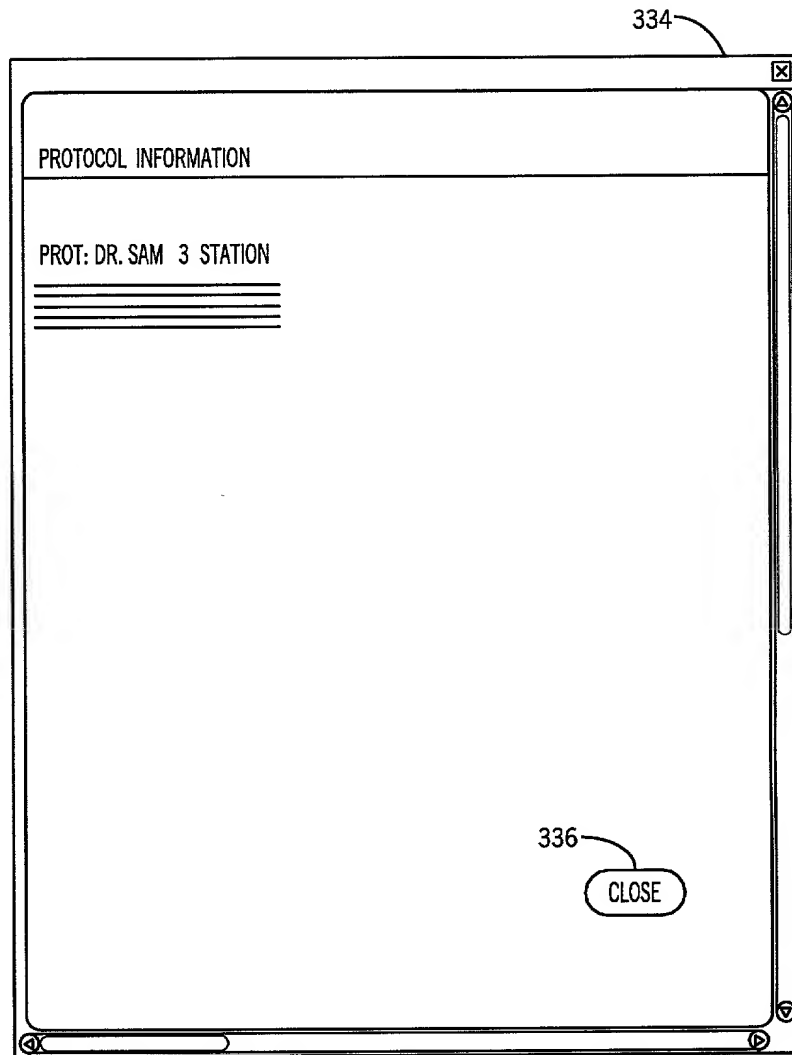


FIG. 16

